



Application Note AN-C-196

# Purity quantification of tris(hydroxymethyl)aminomethane (TRIS) with IC

## Robust analysis with non-suppressed ion chromatography

Tris(hydroxymethyl)aminomethane (also known as TRIS, THAM, or tromethamine) is a common component of buffer solutions in the life sciences. It has a high buffering capacity between pH 7.2–9.0, a pK<sub>a</sub> of 8.2 (20 °C), and complexes with metal ions, making TRIS ideal for biochemistry and molecular biology applications [1]. TRIS buffers are used for DNA purification, separation of proteins with SDS-PAGE

(sodium dodecyl sulfate–polyacrylamide gel electrophoresis), or separation of nucleic acids with gel electrophoresis [2]. TRIS is also used to treat metabolic acidosis and can penetrate the cell membrane in its unionized form, therefore functioning as an intracellular buffer [3]. For these reasons, it is essential to control the purity of TRIS, especially for use in the pharmaceutical industry.

A robust isocratic ion chromatography (IC) method with a Metrosep C Supp 2 - 250/4.0 column and a methanesulfonic acid (MSA) eluent is ideally suited to determine TRIS and any cationic impurities. The microbore IC system (MB) is equipped with the IC

Conductivity Detector MB which is both sensitive and stable against MSA eluents. This guarantees low void volumes, long-term stability of the analytical system, and precise results for TRIS quantification.

## SAMPLE AND SAMPLE PREPARATION

Samples were prepared from Trizma® base (TRIS) powder with p.a. quality (CAS 77-86-1, purchased from Sigma Aldrich No. 93350). For method

evaluation, two different concentrations of TRIS (10.37 mg/L and 103.7 mg/L) were dissolved in eluent (0.1% methanesulfonic acid).


## EXPERIMENTAL

The microbore ion chromatograph 930 Compact IC Flex Oven/DEG/MB was equipped with the MSA-stable IC Conductivity Detector MB (**Figure 1**). An eluent consisting of 0.1% (v/v) MSA (15 mmol/L MSA) was used for this non-suppressed setup (**Table 1**). Samples were injected using the Metrohm intelligent Partial Loop Injection Technique (MiPT, **Figure 2**). This technique fills the 250 µL sample loop with a precisely measured and freely selectable volume (from 5 to 40 µL in this application study). During this process, a Dosino with a 2 mL Dosing Unit performs the precise dosing increments. MiPT enables calibration from a single standard, which was performed here in a range of 5–140 mg/L TRIS.

The variable volume selection can also be applied to sample injection. In such situations, a small injection volume is selected, e.g., for a highly concentrated sample therefore omitting the manual dilution step. Typical inorganic cations (i.e., lithium, sodium, potassium, magnesium, and calcium) were injected on the Metrosep C Supp 2 column to check for potential co-elution issues.



**Figure 1.** The IC Conductivity Detector MB shown here has a reduced cell volume and is inert against methanesulfonic acid.

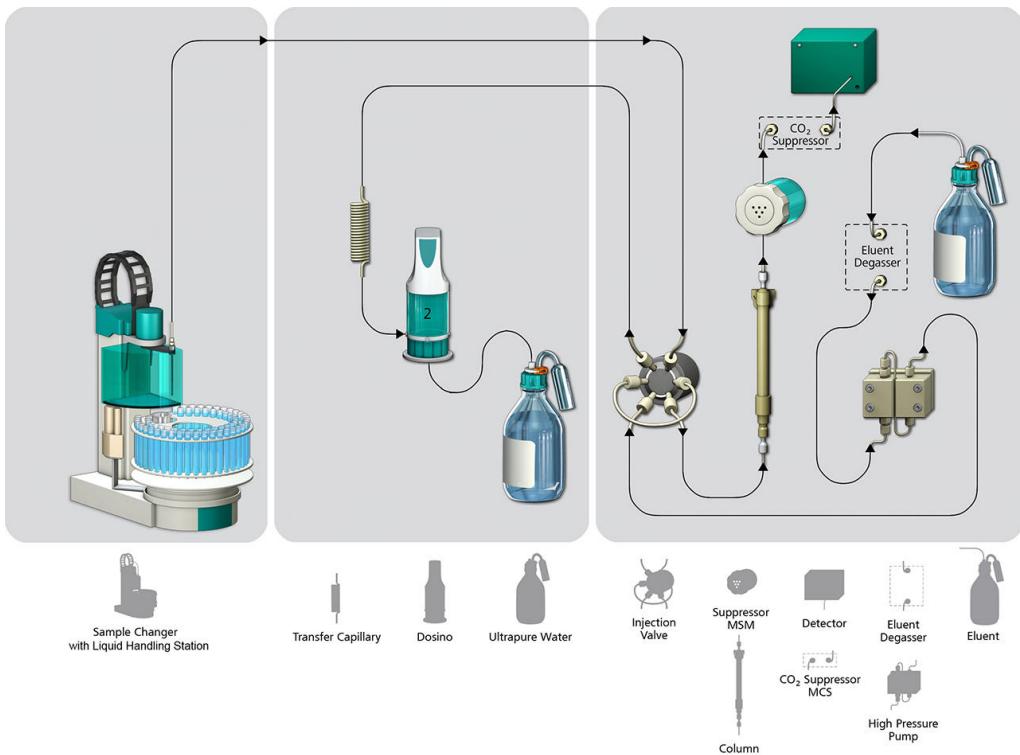

**Figure 2.** Illustration of the Metrohm intelligent Partial Loop Injection Technique (MiPT) flow path. With the help of the Dosino, the sample is transferred from the autosampler into a buffer loop to avoid contamination and carryover. The Dosino then precisely fills the sample loop with the desired injection volume in the  $\mu\text{L}$  range.


**Table 1.** IC method parameters for the microbore IC analysis of cationic impurities in TRIS.

Column	Metrosep C Supp 2 - 250/4.0
Eluent/diluent	c(MSA) = 0.1 % (v/v)
Flow rate	1.0 mL/min
Temperature	30 °C
Injection volume	5–40 $\mu\text{L}$ (MiPT)
Detection	Direct conductivity

## RESULTS

TRIS determination is carried out in less than 8 min using isocratic elution on the MB IC system. The method was proven to be interference-free with regard to major cations as described above.

Sodium had a retention time of 4.1 minutes. Changing the method parameters, e.g., decreasing the column temperature to 20 °C, will increase the resolution between sodium and TRIS. With the used method parameters (**Table 1**), precise determination is possible by using the peak height for evaluation. The recovery rates for 100 mg/L TRIS were 99–103% with a relative standard deviation of <3%, revealing the accuracy of this method.

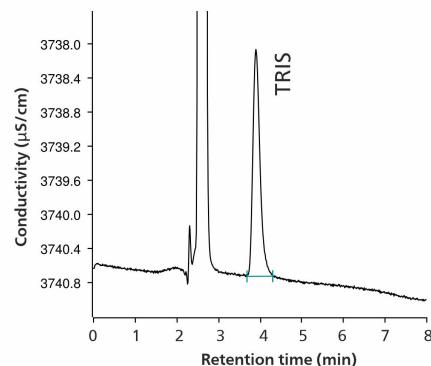

**Figure 3.** Chromatogram of 100 mg/L TRIS with 4 μL injection volume (MiPT).

## CONCLUSION

Raw materials used in the pharmaceutical industry like solutions and buffers must fulfill the highest quality standards with respect to their exact concentration and purity.

The setup in this application study comprises a microbore IC system, an MSA-stable conductivity

detector, and MiPT for automatic calibration with a single standard and flexible choice of sample injection volumes. The method is suitable for the quantification of TRIS in the range of 5–200 mg/L. It guarantees robust determination of the common buffer component TRIS in an easy and precise way.

## REFERENCES

1. Deutscher, M. P. *Guide to Protein Purification*; Gulf Professional Publishing, 1990.
2. Westermeier, R. *Electrophoresis in Practice: A Guide to Methods and Applications of DNA and Protein Separations*; John Wiley & Sons, 2016.
3. Sirieix, D.; Delayance, S.; Paris, M.; et al. Tris-Hydroxymethyl Aminomethane and Sodium Bicarbonate to Buffer Metabolic Acidosis in an Isolated Heart Model. *Am J Respir Crit Care Med* **1997**, *155* (3), 957–963.  
<https://doi.org/10.1164/ajrccm.155.3.9117032>.

## CONTACT

Metrohm France  
13, avenue du Québec - CS  
90038  
91978 VILLEBON  
COURTABOEUF CEDEX

info@metrohm.fr

## CONFIGURATION



### 930 Compact IC Flex Oven/SeS/PP/Deg/MB

Le 930 Compact IC Flex Oven/SeS/PP/Deg est l'appareil CI compact intelligent avec **four à colonne**, **suppression séquentielle** et une **pompe péristaltique** pour la régénération du suppresseur et un **dégazeur** intégré. L'appareil peut être utilisé avec n'importe quelles méthodes de séparation et de détection.

Domaines d'application typiques :

- Déterminations d'anions ou de cations avec suppression séquentielle et détection de conductivité
- Optimisé pour les applications microbores (2 mm), convient parfaitement aux techniques de couplage (IC-MS ou IC-ICP/MS)

Pris en charge avec MagIC Net 4.1 et supérieur



### IC Conductivity Detector MB

Détecteur de conductivité haute performance compact et intelligent destiné aux appareils CI intelligents. Optimisé pour les colonnes microbores. Excellente constance de la température, tout le traitement du signal au sein du bloc de détecteur protégé et DSP – Digital Signal Processing – de la dernière génération garantissent une précision de mesure optimale. Grâce à la plage de travail dynamique, aucun changement de plage n'est nécessaire (même automatique).

#### Domaines d'application typiques :

- Déterminations d'anions ou de cations avec suppression chimique, suppression séquentielle ou sans suppression et détection de conductivité
- Optimisé pour les applications microbores (2 mm), convient parfaitement aux techniques de couplage (IC-MS ou IC-ICP/MS)

#### Spécifications en un coup d'œil :

- 0 à 15 000  $\mu\text{S}/\text{cm}$  sans changement de gamme
- Volume de cellule : 0,3  $\mu\text{L}$
- Électrodes en forme d'anneau en acier inoxydable X2CrNiMo17-12-2 (316 L), compatible MSA
- Pression de fonctionnement maximale : 10,0 MPa (100 bar)
- Température de la cellule : 20 à 50 °C en pas de 5 °C
- Stabilité de la température : < 0,001 °C
- Bruit des lignes de base : < 0,2 nS/cm caractéristique pour la suppression séquentielle
- Capillaires : ID 0,18 mm

Pris en charge avec MagIC Net 4.1 et supérieur



#### Metrosep C Supp 2 - 250/4,0

La colonne de séparation la plus longue de la famille Metrosep C Supp 2 est la Metrosep C Supp 2 - 250/4,0. Le matériau de séparation de la Metrosep C Supp 2 est basé sur un copolymère de polystyrène-divinylbenzène avec groupes carboxyles. Du fait de la séparation optimisée du sodium/ammonium de ce matériau de séparation, cette colonne est idéale pour les déterminations de concentrations d'ammonium infimes accompagnées d'une grande quantité de sodium. La colonne est utilisée avec une suppression séquentielle. Elle est par conséquent particulièrement adaptée à la détermination de concentrations dans la plage moyenne des µg/L et inférieures.