



Application Note AN-V-222

# Iron determination in drinking water

## Wide linear range with a low detection limit using the Bi drop electrode and the triethanolamine method

The presence of iron in drinking water can lead to an unpleasant, harsh metallic taste or reddish-brown stains. In addition, «iron bacteria» which can grow in waters containing Fe as low as 0.1 mg/L, create a reddish-brown slime that can clog plumbing and cause an offensive odor. Over a longer period, the formation of insoluble iron deposits is problematic in many industrial and agricultural applications, such as water supply, system cooling, or field irrigation. To avoid these problems, the U.S. Environmental Protection Agency (EPA) defines the Secondary Maximum Contaminant Level (SMCL) for water

treatment and processing plants as 0.3 mg/L Fe in drinking water.

The voltammetric determination of the iron triethanolamine complex on the non-toxic Bi drop electrode does not require enrichment. This system uses catalytic signal enhancement, allowing both the detection at very low levels (limit of detection of 0.005 mg/L) and measurements in a wide range of concentrations up to 0.5 mg/L. This method is best suited for automated systems or process analyzers, allowing fully automatic determination of iron in a large sample series.

## SAMPLE

Drinking water, mineral water, sea water

## EXPERIMENTAL

The water sample and the supporting electrolyte are pipetted into the measuring vessel. The determination of iron is carried out with a 884 Professional VA using the parameters specified in **Table 1**. The concentration

is determined by two additions of an iron standard addition solution.

The Bi drop electrode is electrochemically activated prior to the first determination.



**Figure 1.** 884 Professional VA fully automated for VA

**Table 1.** Parameters

Parameter	Setting
Mode	DP – Differential Pulse
Start potential	-0.75 V
End potential	-1.25 V
Peak potential Fe	-1 V


## ELECTRODES

- Working electrode: Bi drop
- Reference electrode: Ag/AgCl/KCl (3 mol/L)
- Auxiliary electrode: Glassy carbon rod

## RESULTS

The method is suitable for the determination of iron in water samples in concentrations from  $\beta(\text{Fe}) = 10\text{--}500$

$\mu\text{g/L}$ . The limit of detection of the method is approximately  $\beta(\text{Fe}) = 5 \mu\text{g/L}$ .

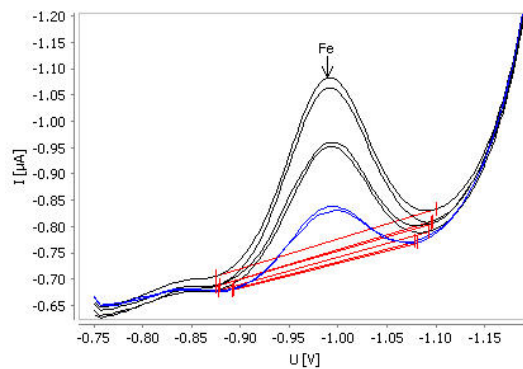

**Figure 2.** Determination of iron in tap water spiked with  $\beta(\text{Fe}) = 20 \mu\text{g/L}$

**Table 2.** Result

Sample	Fe ( $\mu\text{g/L}$ )
Tap water spiked with $\beta(\text{Fe}) = 20 \mu\text{g/L}$	19.1

## REFERENCES

Application Bulletin 439: [Voltammetric determination of iron in water samples with a Bi drop electrode](#)

## CONTACT

Metrohm Indonesia  
Menara Batavia  
10220 Jakarta Pusat

[sales@metrohm.co.id](mailto:sales@metrohm.co.id)

## CONFIGURATION



### 884 Professional VA manual for Multi-Mode Electrode (MME)

884 Professional VA manual for Multi-Mode Electrode (MME) is the entry-level instrument for high-end trace analysis with voltammetry and polarography with the Multi-Mode Electrode pro or the scTRACE Gold or the Bismuth drop electrode. The proven Metrohm electrode methods in combination with a high-performance potentiostat/galvanostat and the extremely flexible viva software open up new perspectives for the determination of heavy metals. The potentiostat with a certified calibrator readjusts itself automatically before each measurement, thus guaranteeing maximum precision.

Determinations with rotating disc electrodes can also be performed with the instrument, e.g. determinations of organic additives in electroplating baths with "Cyclic Voltammetric Stripping" (CVS), "Cyclic Pulse Voltammetric Stripping" (CPVS), and chronopotentiometry (CP). The replaceable measuring head enables rapid changes between the various applications with different electrodes.

The **viva** software is required for control, data collection, and evaluation.

The 884 Professional VA manual for MME is supplied with extensive accessories and a measuring head for the Multi-Mode Electrode pro. Electrode set and **viva** license need to be ordered separately.



### VA electrode equipment with bismuth drop electrode for Professional VA instruments

Complete electrode set for voltammetric determinations of heavy metals. Contains bismuth drop electrode, reference electrode, glassy carbon auxiliary electrode, measuring vessel, stirrer, electrolyte solution, and additional accessories.